



The World Leader in Vibrating Wire Technology

48 Spencer Street
Lebanon, NH 03766, USA
Tel: 603•448•1562
Fax: 603•448•3216
E-mail: geokon@geokon.com
<http://www.geokon.com>

Instruction Manual

Model 4450

VW Displacement Transducer



No part of this instruction manual may be reproduced, by any means, without the written consent of Geokon, Inc.

The information contained herein is believed to be accurate and reliable. However, Geokon, Inc. assumes no responsibility for errors, omissions or misinterpretation. The information herein is subject to change without notification.

Copyright © 1994, 1996, 2004, 2008 by Geokon, Inc.
(Doc Rev K, 9/08)

Warranty Statement

Geokon, Inc. warrants its products to be free of defects in materials and workmanship, under normal use and service for a period of 13 months from date of purchase. If the unit should malfunction, it must be returned to the factory for evaluation, freight prepaid. Upon examination by Geokon, if the unit is found to be defective, it will be repaired or replaced at no charge. However, the WARRANTY is VOID if the unit shows evidence of having been tampered with or shows evidence of being damaged as a result of excessive corrosion or current, heat, moisture or vibration, improper specification, misapplication, misuse or other operating conditions outside of Geokon's control. Components which wear or which are damaged by misuse are not warranted. This includes fuses and batteries.

Geokon manufactures scientific instruments whose misuse is potentially dangerous. The instruments are intended to be installed and used only by qualified personnel. There are no warranties except as stated herein. There are no other warranties, expressed or implied, including but not limited to the implied warranties of merchantability and of fitness for a particular purpose. Geokon, Inc. is not responsible for any damages or losses caused to other equipment, whether direct, indirect, incidental, special or consequential which the purchaser may experience as a result of the installation or use of the product. The buyer's sole remedy for any breach of this agreement by Geokon, Inc. or any breach of any warranty by Geokon, Inc. shall not exceed the purchase price paid by the purchaser to Geokon, Inc. for the unit or units, or equipment directly affected by such breach. Under no circumstances will Geokon reimburse the claimant for loss incurred in removing and/or reinstalling equipment.

Every precaution for accuracy has been taken in the preparation of manuals and/or software, however, Geokon, Inc. neither assumes responsibility for any omissions or errors that may appear nor assumes liability for any damages or losses that result from the use of the products in accordance with the information contained in the manual or software.

TABLE of CONTENTS

	Page
1. INTRODUCTION	1
1.1. THEORY OF OPERATION	1
2. INSTALLATION	1
2.1. PRELIMINARY TESTS	1
2.2. DISPLACEMENT TRANSDUCER INSTALLATION.....	1
2.3. CABLE INSTALLATION	2
2.4. ELECTRICAL NOISE.....	2
2.5. INITIAL READINGS.....	2
2.6. LIGHTNING PROTECTION	2
3. TAKING READINGS.....	3
3.1. OPERATION OF THE GK-401 READOUT BOX	3
3.2. OPERATION OF THE GK-403 READOUT BOX	3
3.3. OPERATION OF THE GK-404 READOUT BOX	4
3.4. MEASURING TEMPERATURES	4
4. DATA REDUCTION	4
4.1. DISPLACEMENT CALCULATION	4
4.2. TEMPERATURE CORRECTION	5
4.3. ENVIRONMENTAL FACTORS.....	6
5. TROUBLESHOOTING.....	7
APPENDIX A - SPECIFICATIONS	8
A.1. MODEL 4450 DISPLACEMENT TRANSDUCER	8
A.2. THERMISTOR (SEE APPENDIX B ALSO).....	8
APPENDIX B - THERMISTOR TEMPERATURE DERIVATION	9

LIST of FIGURES, TABLES and EQUATIONS

	Page
FIGURE 1 - MODEL 4450 DISPLACEMENT TRANSDUCER	1
TABLE 1 - MODEL 4450 READING VERSUS POSITION IN THE RANGE	2
FIGURE 2 - LIGHTNING PROTECTION SCHEME	3
EQUATION 1 - DIGITS CALCULATION.....	5
EQUATION 2 - DISPLACEMENT CALCULATION.....	5
TABLE 2 - ENGINEERING UNITS CONVERSION MULTIPLIERS	5
EQUATION 3 - THERMALLY CORRECTED DISPLACEMENT CALCULATION.....	5
EQUATION 4 - THERMAL COEFFICIENT CALCULATION	6
TABLE 3 - THERMAL COEFFICIENT CALCULATION CONSTANTS	6
TABLE A-1 MODEL 4450 DISPLACEMENT TRANSDUCER SPECIFICATIONS.....	8
EQUATION B-1 CONVERT THERMISTOR RESISTANCE TO TEMPERATURE.....	9
TABLE B-1 THERMISTOR RESISTANCE VERSUS TEMPERATURE	9

1. INTRODUCTION

1.1. Theory of Operation

The instrument consists of a vibrating wire sensing element in series with a heat treated, stress relieved spring which is connected to the wire at one end and a connecting rod at the other. The unit is fully sealed and operates at pressures of up to 250 psi. As the connecting rod is pulled out from the gage body, the spring is elongated causing an increase in tension which is sensed by the vibrating wire element. The tension in the wire is directly proportional to the extension, hence, the change in displacement can be determined very accurately by measuring the strain change with the vibrating wire readout box.

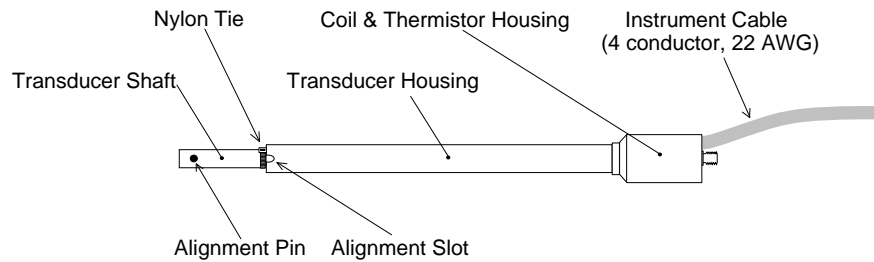


Figure 1 - Model 4450 Displacement Transducer

CAUTION: Do not rotate the shaft of the Displacement Transducer. This may cause irreparable damage to the instrument. The alignment pin on the transducer shaft and slot on the body serve as a guide for alignment.

2. INSTALLATION

2.1. Preliminary Tests

Upon receipt of the instrument, the gage should be checked for proper operation (including the thermistor **The Displacement Transducer normally arrives with it's shaft secured at approximately 50% of it's range, by either a split PVC sleeve, (for transducers over 100mm (4 inch) range), or a nylon Tyrap, (see Figure 1).** This holds the instrument in tension thereby helping protect it during shipping. **Remove this PVC split sleeve or Tyrap before proceeding.** Connect the gage to the Readout to take a reading (see section 3). The reading should be stable and in the range of 4000 to 5000. When the nylon tie is removed the reading should be in the range of 2000 to 3000 when the alignment pin rests on the housing tube (see Figure 1).

When pulling the transducer shaft out to check for proper operation do not extend the shaft more than the range of the gage!

Checks of electrical continuity can also be made using an ohmmeter. Resistance between the gage leads should be approximately 180Ω , $\pm 10\Omega$. Remember to add cable resistance when checking (22 AWG stranded copper leads are approximately $14.7\Omega/1000'$ or $48.5\Omega/km$, multiply by 2 for both directions). Between the green and white should be approximately 3000 ohms at 25° (see Table B-1), and between any conductor and the shield should exceed 2 megohms.

2.2. Displacement Transducer Installation

1. Place the transducer shaft pin into the transducer tube slot first, to prevent twisting the internal vibrating wire during installation.
2. Rotate the transducer approximately 16 turns to tighten the transducer shaft, with its #10-32 thread, against the shaft mounting device.

3. Attach the red and black gage leads to the readout box. Select readout in digits (position "B", see section 3).
4. Gently pull the gage tube, allowing the tube notch to extend away from the shaft pin until the desired reading is obtained (see Table 1).
5. Hold the desired reading and secure the cable side of the gage against or* inside the mounting device. Do not rotate the gage tube relative to the shaft while securing. Note: The transducer may be damaged if its allowed to free-fall through its stroke. (*The transducer can be secured by using a Swagelok male connector with nylon front and back ferrules, tightened one full turn beyond fingertight.)

Transducer	Digit Change	Minimum Reading	Maximum Reading	Mid-Range	1/3 Compression 1/3 Extension	1/3 Extension 1/3 Compression
Standard 12, 25, 50 mm	5,000	2000	7000	5000	6500	4000
Slim 12, 25, 50 mm	10,000	3000	13000	8000	6000	9000
Standard 100, 150 mm	5,000	2000	7000	5000	6500	4000

Table 1 - Model 4450 Reading versus Position in the Range

2.3. Cable Installation

The cable should be routed in such a way so as to minimize the possibility of damage due to moving equipment, debris or other causes.

Cables may be spliced to lengthen them, without affecting gage readings. Always waterproof the splice completely, preferably using an epoxy based splice kit such the 3M Scotchcast™, model 82-A1. These kits are available from the factory.

2.4. Electrical Noise

Care should be exercised when installing instrument cables to keep them as far away as possible from sources of electrical interference such as power lines, generators, motors, transformers, arc welders, etc. Cables should never be buried or run with AC power lines. The instrument cables will pick up the 50 or 60 Hz (or other frequency) noise from the power cable and this will likely cause a problem obtaining a stable reading. Contact the factory concerning filtering options available for use with the Geokon dataloggers and readouts should difficulties arise.

2.5. Initial Readings

Initial readings must be taken and carefully recorded along with the temperature at the time of installation. These readings serve as a reference for subsequent deformation calculations.

2.6. Lightning Protection

The Model 4450 Vibrating Wire Displacement Transducers, unlike numerous other types of instrumentation available from Geokon, do not have any integral lightning protection components, i.e. transzorb or plasma surge arrestors. Usually this is not a problem however, if the instrument cable is exposed, it may be appropriate to install lightning protection components, as the transient could travel down the cable to the gage and possibly destroy it.

Note the following suggestions;

- If the gage is connected to a terminal box or multiplexer components such as plasma surge arrestors (spark gaps) may be installed in the terminal box/multiplexer to provide a measure of transient protection.

Terminal boxes and multiplexers available from Geokon provide locations for installation of these components.

- Lighting arrestor boards and enclosures are available from Geokon that install near the instrument. The enclosure has a removable top so, in the event the protection board (LAB-3) is damaged, the user may service the components (or replace the board). A connection is made between this enclosure and earth ground to facilitate the passing of transients away from the gage. See Figure 2. Consult the factory for additional information on these or alternate lightning protection schemes.
- Plasma surge arrestors can be epoxy potted into the gage cable close to the sensor. A ground strap would connect the surge arrestor to earth ground, either a grounding stake or other suitable earth ground such as perhaps the strand to which the transducer is attached.

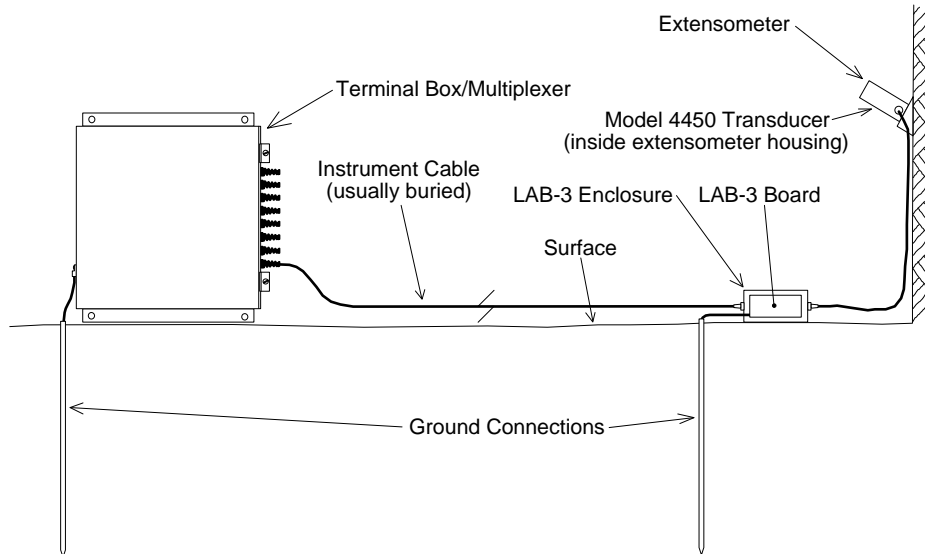


Figure 2 - Lightning Protection Scheme

3. TAKING READINGS

3.1. Operation of the GK-401 Readout Box

The GK-401 is a basic readout for all Vibrating Wire Displacement Transducers.

Connect the Readout using the flying leads or in the case of a terminal station, with a connector. The red and black clips are for the vibrating wire transducer, the green or blue clip for the shield drain wire. The GK-401 cannot read the thermistor (see Section 3.4).

1. Turn on the Readout. Turn the display selector to position "B". Readout is in "digits" (see Equation 1).
2. Turn the unit on and a reading will appear in the front display window. The last digit may change one or two digits while reading. Record the value displayed. If zeros are displayed or the reading is unstable see section 5 for troubleshooting suggestions.
3. The unit will automatically turn itself off after approximately 4 minutes to conserve power.

3.2. Operation of the GK-403 Readout Box

The GK-403 can store gage readings and also apply calibration factors to convert readings to engineering units. Consult the GK-403 Instruction Manual for additional information on Mode "G" of the Readout. The following instructions will explain taking gage measurements using Mode "B".

Connect the Readout using the flying leads or in the case of a terminal station, with a connector. The red and black clips are for the vibrating wire transducer, the white and green clips are for the thermistor and the blue for the shield drain wire.

1. Turn on the Readout. Turn the display selector to position "B". Readout is in digits (see Equation 1).
2. Turn the unit on and a reading will appear in the front display window. The last digit may change one or two digits while reading. Press the "Store" button to record the value displayed. If the no reading displays or the reading is unstable see section 5 for troubleshooting suggestions. The thermistor will be read and output directly in degrees centigrade.
3. The unit will automatically turn itself off after approximately 2 minutes to conserve power.

3.3 Operation of the GK-404 Readout Box

The GK-404 is a palm sized readout box which displays the Vibrating wire value and the temperature in degrees centigrade.

The GK-404 Vibrating Wire Readout arrives with a patch cord for connecting to the vibrating wire gages. One end will consist of a 5-pin plug for connecting to the respective socket on the bottom of the GK-404 enclosure. The other end will consist of 5 leads terminated with alligator clips. Note the colors of the alligator clips are red, black, green, white and blue. The colors represent the positive vibrating wire gage lead (red), negative vibrating wire gage lead (black), positive thermistor lead (green), negative thermistor lead (white) and transducer cable drain wire (blue). The clips should be connected to their respectively colored leads from the vibrating wire gage cable.

Use the **POS** (Position) button to select position **B** and the **MODE** button to select **Dg** (digits).

Other functions can be selected as described in the GK404 Manual.

The GK-404 will continue to take measurements and display the readings until the **OFF** button is pushed, or if enabled, when the automatic Power-Off timer shuts the GK-404 off.

The GK-404 continuously monitors the status of the (2) 1.5V AA cells, and when their combined voltage drops to 2V, the message **Batteries Low** is displayed on the screen. A fresh set of 1.5V AA batteries should be installed at this point

3.4. Measuring Temperatures

Each Vibrating Wire Displacement Transducer is equipped with a thermistor for reading temperature. The thermistor gives a varying resistance output as the temperature changes. Usually the white and green leads are connected to the internal thermistor. The GK-401 Readout Box does not read temperatures – a digital ohmmeter is required. The GK-403 and GK 404 readout boxes will read the thermistor and display temperature in °C automatically

1. Connect the ohmmeter to the two thermistor leads coming from the transducer. (Since the resistance changes with temperature are so large, the effect of cable resistance is usually insignificant.)
2. Look up the temperature for the measured resistance in Table B-1 (Appendix B). Alternately the temperature could be calculated using Equation B-1 (Appendix B). For example, a resistance of 3400 ohms equivalent to 22° C. When long cables are used the cable resistance may need to be taken into account. Standard 22 AWG stranded copper lead cable is approximately 14.7Ω/1000' or 48.5Ω/km, multiply by 2 for both directions.

4. DATA REDUCTION

4.1. Displacement Calculation

The basic units utilized by Geokon for measurement and reduction of data from Vibrating Wire Displacement Transducers are "digits". Calculation of digits is based on the following equation;

$$\text{Digits} = \left(\frac{1}{\text{Period}} \right)^2 \times 10^{-3} \quad \text{or} \quad \text{Digits} = \frac{\text{Hz}^2}{1000}$$

Equation 1 - Digits Calculation

To convert digits to displacement the following equation applies;

$$D_{\text{uncorrected}} = (R_1 - R_0) \times G$$

Equation 2 - Displacement Calculation

Where; R_1 is the current reading.
 R_0 is the initial reading, usually obtained at installation (see section 2.4).
 G is the calibration factor, usually millimeters or inches per digit.

For example, the initial reading, R_0 , at installation of a displacement transducer is 6783 digits. The current reading, R_1 , is 7228. The calibration factor, G , is 0.011906 mm/digit. The deformation change is;

$$D_{\text{uncorrected}} = (7228 - 6783) \times 0.011906 = +5.3 \text{ mm}$$

Note that increasing readings (digits) indicate increasing extension.

To convert to other engineering units refer to Table 2

From→ To↓	Inches	Feet	Millimeters	Centimeters	Meters
Inches	1	12	0.03937	0.3937	39.37
Feet	0.0833	1	0.003281	0.03281	3.281
Millimeters	25.4	304.8	1	10	1000
Centimeters	2.54	30.48	0.10	1	100
Meters	0.0254	0.3048	0.001	0.01	1

Table 2 - Engineering Units Conversion Multipliers

4.2. Temperature Correction

The Model 4450 Vibrating Wire Displacement Transducers have a small coefficient of thermal expansion so in many cases correction may not be necessary. However, if maximum accuracy is desired or the temperature changes are extreme (>10° C) corrections may be applied.

The following equation applies;

$$D_{\text{corrected}} = ((R_1 - R_0) \times G) + ((T_1 - T_0) \times K)$$

Equation 3 - Thermally Corrected Displacement Calculation

Where: R_1 is the current reading.
 R_0 is the initial reading.
 G is the calibration Factor.
 T_1 is the current temperature.
 T_0 is the initial temperature.
 K is the thermal coefficient (see Equation 4).

Tests have determined that the thermal coefficient, K, changes with the position of the transducer shaft. Hence, the first step in the temperature correction process is determination of the proper thermal coefficient based on the following equation;

$$K = ((R_1 \times TM) + TB) \times G$$

Equation 4 - Thermal Coefficient Calculation

Where: R_1 is the current reading.
 TM is the multiplier from Table 3.
 TB is the constant from Table 3.
 G is the calibration factor, usually millimeters or inches per digit.

Model:	4450-12 mm 4450-0.5"	4450-25 mm 4450-1"	4450-50 mm 4450-2"	4450-100 mm 4450-4"	4450-150 mm 4450-6"
Multiplier (TM):	0.000295	0.000301	0.000330	0.000192	0.000216
Constant (TB):	1.724	0.911	0.415	0.669	0.491

Model:	4450-200mm 4450-8.0"	4450-300mm 4450-12"			
Multiplier (TM):	0.000305	0.000245			
Constant (TB):	0.240	0.564			

Table 3 - Thermal Coefficient Calculation Constants

Consider the following example using a Model 4450-50 mm Displacement Transducer;

$$R_0 = 6783 \text{ digits}$$

$$R_1 = 7228 \text{ digits}$$

$$T_0 = 15.8^\circ C$$

$$T_1 = 27.2^\circ C$$

$$G = 0.011906 \text{ mm/digit}$$

$$K = ((7228 \times 0.000330) + 0.415) \times 0.011906 = 0.0333$$

$$D_{corrected} = ((R_1 - R_0) \times C) + ((T_1 - T_0) \times K)$$

$$D_{corrected} = ((7228 - 6783) \times 0.011906) + ((27.2 - 15.8) \times 0.0333)$$

$$D_{corrected} = (445 \times 0.011906) + 0.380$$

$$D_{corrected} = 5.298 + 0.380$$

$$D_{corrected} = 5.678 \text{ mm}$$

4.3. Environmental Factors

Since the purpose of the displacement transducer installation is to monitor site conditions, factors which may affect these conditions should always be observed and recorded. Seemingly minor effects may have a real influence on the behavior of the structure being monitored and may give an early indication of potential problems. Some of these factors include, but are not limited to: blasting, rainfall, tidal levels, excavation and fill levels and sequences, traffic, temperature and barometric changes, changes in personnel, nearby construction activities, seasonal changes, etc.

5. TROUBLESHOOTING

Consult the following list of problems and possible solutions should difficulties arise. Consult the factory for additional troubleshooting help.

Symptom: Displacement Transducer Readings are Unstable

- ✓ Is the readout box position set correctly? If using a datalogger to record readings automatically are the swept frequency excitation settings correct? Try reading the displacement transducer on a different readout position. For instance, channel A of the GK-401 and GK-403 might be able to read the transducer. To convert the Channel A period display to digits use Equation 1.
- ✓ Is there a source of electrical noise nearby? Most probable sources of electrical noise are motors, generators, transformers, arc welders and antennas. Make sure the shield drain wire is connected to ground whether using a portable readout or datalogger. If using the GK-401 Readout connect the clip with the green boot to the bare shield drain wire of the pressure cell cable. If using the GK-403 connect the clip with the blue boot to the shield drain wire.
- ✓ Does the readout work with another displacement transducer? If not, the readout may have a low battery or be malfunctioning. Consult the appropriate readout manual for charging or troubleshooting directions.
- ✓ Has the transducer gone outside its range? If so, the transducer can be reset using the installation instructions in section 2.

Symptom: Displacement Transducer Fails to Read

- ✓ Is the cable cut or crushed? This can be checked with an ohmmeter. Nominal resistance between the two gage leads (usually red and black leads) is $180\Omega, \pm 10\Omega$. Remember to add cable resistance when checking (22 AWG stranded copper leads are approximately $14.7\Omega/1000'$ or $48.5\Omega/\text{km}$, multiply by 2 for both directions). If the resistance reads infinite, or very high (megohms), a cut wire must be suspected. If the resistance reads very low ($<100\Omega$) a short in the cable is likely.
- ✓ Does the readout or datalogger work with another transducer? If not, the readout or datalogger may be malfunctioning. Consult the readout or datalogger manual for further direction.

APPENDIX A - SPECIFICATIONS**A.1. Model 4450 Displacement Transducer**

Range:	12 mm 0.50 inches	25 mm 1 inch	50 mm 2 inches	100 mm 4 inches	150 mm 6 inches
Resolution:¹	0.025% FSR				
Linearity:	0.25% FSR				
Thermal Zero Shift:²	< 0.05% FSR/°C				
Stability:	< 0.2%/yr (under static conditions)				
Overrange:	115%				
Temperature Range:	-40 to +80°C -40 to 180° F				
Frequency Range: (standard model)	1200 - 2800 Hz				
Frequency Range: (slim stick model)	1700 - 3600 Hz				
Coil Resistance:	180 Ω, ±10 Ω				
Cable Type:³	2 twisted pair (4 conductor) 22 AWG Foil shield, PVC jacket, nominal OD=6.3 mm (0.250")				

Table A-1 Model 4450 Displacement Transducer Specifications

Notes:

¹ Minimum, greater resolution possible depending on readout.² Depends on application.³ Polyurethane jacket cable available.**A.2 Thermistor (see Appendix B also)**

Range: -80 to +150° C

Accuracy: ±0.5° C

APPENDIX B - THERMISTOR TEMPERATURE DERIVATION

Thermistor Type: YSI 44005, Dale #1C3001-B3, Alpha #13A3001-B3

Resistance to Temperature Equation:

$$T = \frac{1}{A + B(\ln R) + C(\ln R)^3} - 273.2$$

Equation B-1 Convert Thermistor Resistance to Temperature

where: T = Temperature in °C.
 LnR = Natural Log of Thermistor Resistance
 A = 1.4051×10^{-3} (coefficients calculated over the -50 to +150° C. span)
 B = 2.369×10^{-4}
 C = 1.019×10^{-7}

Ohms	Temp	Ohms	Temp	Ohms	Temp	Ohms	Temp	Ohms	Temp
201.1K	-50	16.60K	-10	2417	+30	525.4	+70	153.2	+110
187.3K	-49	15.72K	-9	2317	31	507.8	71	149.0	111
174.5K	-48	14.90K	-8	2221	32	490.9	72	145.0	112
162.7K	-47	14.12K	-7	2130	33	474.7	73	141.1	113
151.7K	-46	13.39K	-6	2042	34	459.0	74	137.2	114
141.6K	-45	12.70K	-5	1959	35	444.0	75	133.6	115
132.2K	-44	12.05K	-4	1880	36	429.5	76	130.0	116
123.5K	-43	11.44K	-3	1805	37	415.6	77	126.5	117
115.4K	-42	10.86K	-2	1733	38	402.2	78	123.2	118
107.9K	-41	10.31K	-1	1664	39	389.3	79	119.9	119
101.0K	-40	9796	0	1598	40	376.9	80	116.8	120
94.48K	-39	9310	+1	1535	41	364.9	81	113.8	121
88.46K	-38	8851	2	1475	42	353.4	82	110.8	122
82.87K	-37	8417	3	1418	43	342.2	83	107.9	123
77.66K	-36	8006	4	1363	44	331.5	84	105.2	124
72.81K	-35	7618	5	1310	45	321.2	85	102.5	125
68.30K	-34	7252	6	1260	46	311.3	86	99.9	126
64.09K	-33	6905	7	1212	47	301.7	87	97.3	127
60.17K	-32	6576	8	1167	48	292.4	88	94.9	128
56.51K	-31	6265	9	1123	49	283.5	89	92.5	129
53.10K	-30	5971	10	1081	50	274.9	90	90.2	130
49.91K	-29	5692	11	1040	51	266.6	91	87.9	131
46.94K	-28	5427	12	1002	52	258.6	92	85.7	132
44.16K	-27	5177	13	965.0	53	250.9	93	83.6	133
41.56K	-26	4939	14	929.6	54	243.4	94	81.6	134
39.13K	-25	4714	15	895.8	55	236.2	95	79.6	135
36.86K	-24	4500	16	863.3	56	229.3	96	77.6	136
34.73K	-23	4297	17	832.2	57	222.6	97	75.8	137
32.74K	-22	4105	18	802.3	58	216.1	98	73.9	138
30.87K	-21	3922	19	773.7	59	209.8	99	72.2	139
29.13K	-20	3748	20	746.3	60	203.8	100	70.4	140
27.49K	-19	3583	21	719.9	61	197.9	101	68.8	141
25.95K	-18	3426	22	694.7	62	192.2	102	67.1	142
24.51K	-17	3277	23	670.4	63	186.8	103	65.5	143
23.16K	-16	3135	24	647.1	64	181.5	104	64.0	144
21.89K	-15	3000	25	624.7	65	176.4	105	62.5	145
20.70K	-14	2872	26	603.3	66	171.4	106	61.1	146
19.58K	-13	2750	27	582.6	67	166.7	107	59.6	147
18.52K	-12	2633	28	562.8	68	162.0	108	58.3	148
17.53K	-11	2523	29	543.7	69	157.6	109	56.8	149
								55.6	150

Table B-1 Thermistor Resistance versus Temperature